


-15kV TOF: -9245 v
 -3.6kV MCP: -2782 v
 -2.4kV MCP: -1579 v
 Input Cur: 294 ma
 RPA max: 237 v
 Mirror max: 238 v

Tue Sep 26 12:21:32 2006

TIDE Direct Events

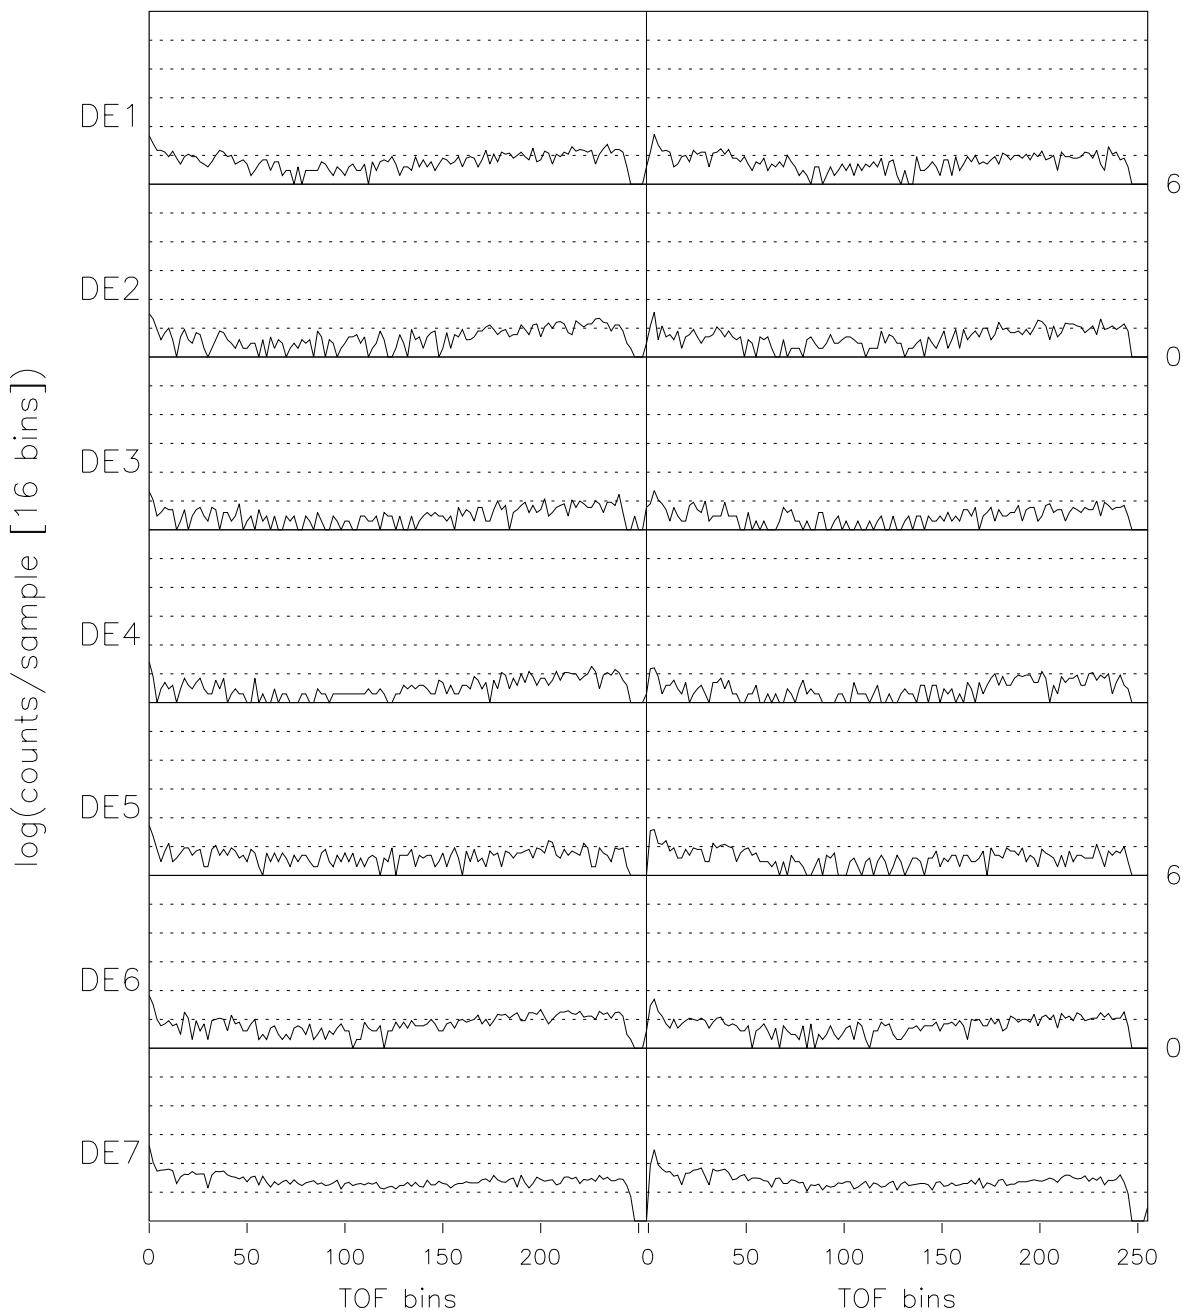

reported: 09-26-96 04:52:13 UT

reported: 09-26-96 04:55:26 UT

file: /export/data/tide/nrt/96092601.dat

-15kV TOF: -9181 v

-3.6kV MCP: -2782 v

-2.4kV MCP: -1579 v

Input Cur: 302 ma

RPA max: 237 v

Mirror max: 238 v